

Tricuspid Valve Replacement

A Percutaneous Transfemoral Valve-in-Ring Approach



Alduz S. Cabasa, MD,* Mackram F. Eleid, MD,† Charanjit S. Rihal, MD,† Hector R. Villarraga, MD,† Thomas A. Foley, MD,‡ Rakesh M. Suri, MD, DPHIL*

We describe a percutaneous transcatheter tricuspid valve-in-ring implantation using the Sapien XT prosthesis (Edward Lifesciences, Irvine, California) (1,2). A 68-year-old woman with rheumatic heart disease and 2 previous sternotomies including tricuspid valve repair with a 32-mm Carpentier-Edwards (Irvine, California) annuloplasty ring presented 2 years prior with severe tricuspid valve regurgitation (annulus dilation and tenting of the leaflet) and pulmonary hypertension (right ventricular systolic pressure of 46 mm Hg) related to left ventricular diastolic dysfunction. After multidisciplinary evaluation, a percutaneous approach was recommended to avoid increased risk of third-time redo sternotomy. The procedure was planned using a cardiac computed tomography-derived 3-dimensional printed model created using an Objet Connex 350 printer (Stratasys, Eden Prairie, Minnesota) (Figure 1). Using this model, the prosthesis size was selected and “test deployed” to verify adequacy (Online Video 1). The actual transcatheter tricuspid valve-in-ring implantation was performed in the hybrid operating suite under general anesthesia. The right

common femoral vein was accessed percutaneously. With an Amplatz super-stiff wire (Boston Scientific, Marlborough, Massachusetts) acting as a rail, a 29-mm Sapien XT valve was advanced across the tricuspid valve annulus. The stented valve was balloon inflated with an additional 1 cc of contrast saline solution to achieve optimal conical deployment (Figure 2, Online Video 2). Transesophageal echocardiography showed only mild perivalvular regurgitation in the septal region, as predicted in the printed model. Post-procedural 2-dimensional echocardiography showed mild tricuspid valve regurgitation with a transvalvular gradient of 3 mm Hg (Figure 3, Online Video 3). The patient’s dyspnea improved prior to discharge from hospital 4 days later. The long-term effectiveness of this off-label procedure is still unknown and warrants further studies.


REPRINT REQUESTS AND CORRESPONDENCE:

Dr. Rakesh M. Suri, Department of Thoracic and Cardiovascular Surgery, Cleveland Clinic Foundation, 9500 Euclid Avenue, J4-1, Cleveland, Ohio 44195. E-mail: surir@ccf.org.

From the *Division of Cardiovascular Surgery, Mayo Clinic College of Medicine, Rochester, Minnesota; †Division of Cardiovascular Diseases, Mayo Clinic College of Medicine, Rochester, Minnesota; and the ‡Department of Radiology, Mayo Clinic College of Medicine, Rochester, Minnesota. Dr. Suri received research support to the Division of Cardiovascular Surgery from Sorin, Abbott Vascular, St. Jude Medical, and Edwards Lifesciences; was a co-primary investigator on behalf of Abbott for the COAPT trial; is the national primary investigator on behalf of Sorin on the Perceval trial; applied for patents in conjunction with Sorin; and served on the steering committees of the COAPT trial for Abbott and the PORTICO trial for St. Jude Medical. All other authors have reported that they have no conflicts of interest relevant to the contents of this paper to disclose. Drs. Cabasa and Eleid contributed equally to this work.


Manuscript received March 6, 2015; accepted March 12, 2015.

FIGURE 1 Pre- and Post-Procedure CT Imaging and 3D Printed Model

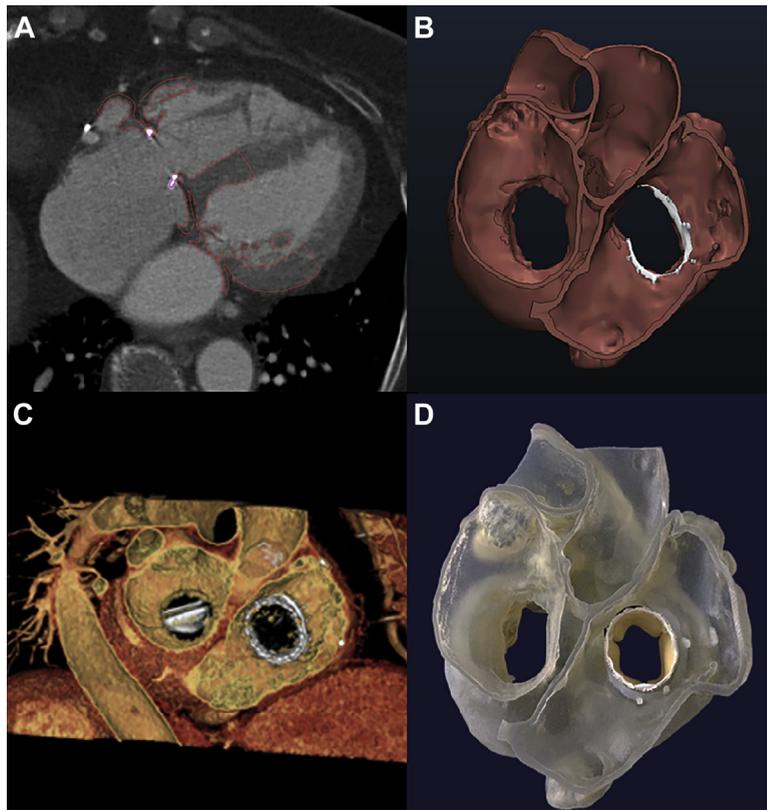


(A) Pre-procedure electrocardiography-gated cardiac computed tomography (CT) scan with the outline of the standard template library files (**red and purple outlines**) used for printing of the 3-dimensional (3D) model projected on the CT image. **(B)** The 3D reconstruction of the standard template library files showing the anatomy included in the printed model. **(C)** Post-operative volume-rendered 3D image showing the implanted Sapien XT valve within the annulus. **(D)** The 3D printed model, which is made up of acrylic-based photopolymer resins of differing stiffness for the annuloplasty band and myocardium. The appropriate size of the Sapien XT valve was pre-operatively determined using the model. See [Online Video 1](#).

FIGURE 2 Fluoroscopy Images of the Procedure

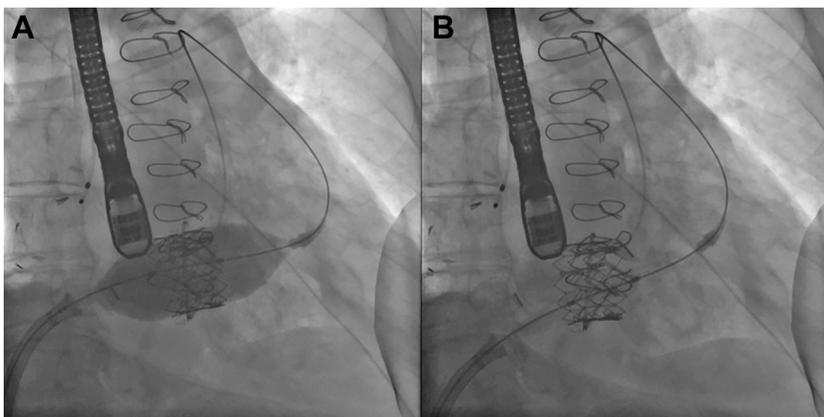

(A) Additional 1 cc of contrast saline solution was used to achieve optimal conical deployment. **(B)** Post-balloon expansion of the Sapien XT valve image showing a well-seated valve with the majority of the stent on the right atrial side of the annulus. See [Online Video 2](#).

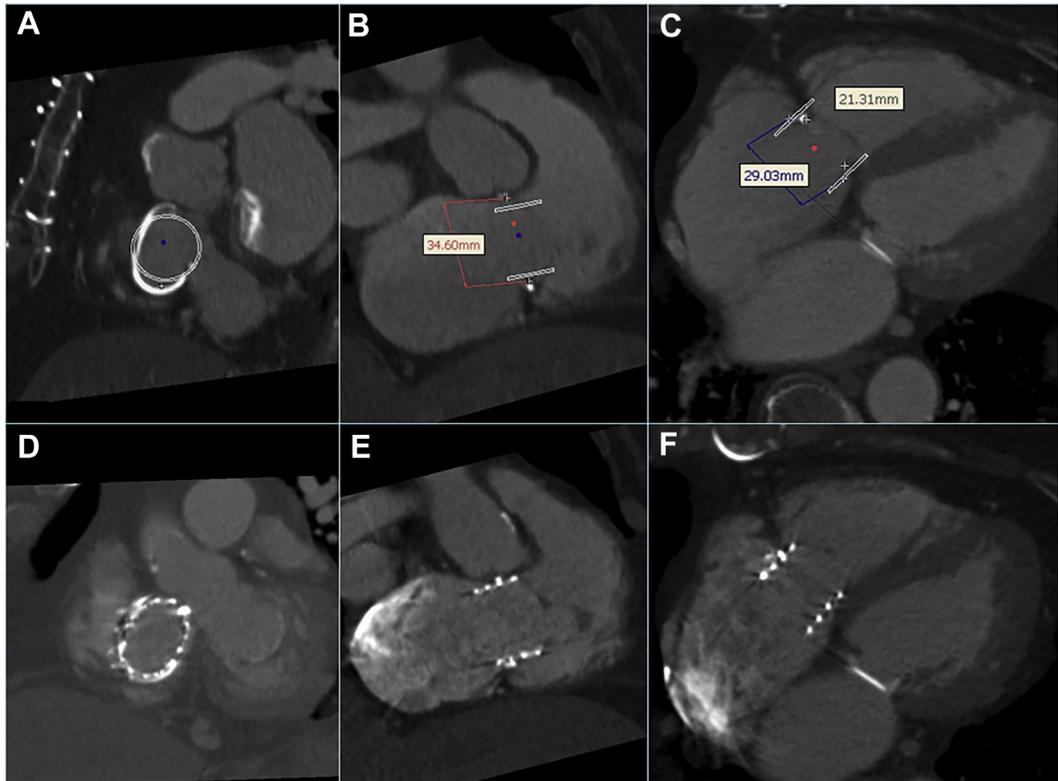FIGURE 3 Virtual Model of Sapien XT Projected on CT Image

Reformatted pre-procedure cardiac computed tomography (CT) images with “virtual” model of the 29-mm Sapien XT valve projected on the CT image in the tricuspid position (**A to C**) and reformatted post-procedure implantation cardiac CT images showing the position of the Sapien valve after implantation (**D to F**). The valve stent appears well opposed to the annulus and annuloplasty band. See [Online Video 3](#).

REFERENCES

1. Hoendermis ES, Douglas YL, van den Heuvel AF. Percutaneous Edwards Sapien valve implantation in the tricuspid position: case report and review of literature. *EuroIntervention* 2012;8:628-33.
2. Raval J, Nagaraja V, Eslick GD, Dennis AR. Transcatheter valve-in-valve implantation: a systemic review of literature. *Heart Lung Circ* 2014; 23:1020-8.

KEY WORDS Sapien XT, transcatheter, tricuspid valve, valve-in-ring

APPENDIX For supplemental videos, please see the online version of this paper.